



## King's Research Portal

DOI:

[10.1161/CIRCINTERVENTIONS.118.007577](https://doi.org/10.1161/CIRCINTERVENTIONS.118.007577)

*Document Version*

Publisher's PDF, also known as Version of record

[Link to publication record in King's Research Portal](#)

*Citation for published version (APA):*

Modi, B. N., Sankaran, S., Kim, H. J., Ellis, H., Rogers, C., Taylor, C. A., Rajani, R., & Perera, D. (2019). Predicting the Physiological Effect of Revascularization in Serially Diseased Coronary Arteries: Clinical validation of a novel CT coronary angiography-based technique. *Circulation. Cardiovascular interventions*, 12(2), Article e007577. <https://doi.org/10.1161/CIRCINTERVENTIONS.118.007577>

### **Citing this paper**

Please note that where the full-text provided on King's Research Portal is the Author Accepted Manuscript or Post-Print version this may differ from the final Published version. If citing, it is advised that you check and use the publisher's definitive version for pagination, volume/issue, and date of publication details. And where the final published version is provided on the Research Portal, if citing you are again advised to check the publisher's website for any subsequent corrections.

### **General rights**

Copyright and moral rights for the publications made accessible in the Research Portal are retained by the authors and/or other copyright owners and it is a condition of accessing publications that users recognize and abide by the legal requirements associated with these rights.

- Users may download and print one copy of any publication from the Research Portal for the purpose of private study or research.
- You may not further distribute the material or use it for any profit-making activity or commercial gain
- You may freely distribute the URL identifying the publication in the Research Portal

### **Take down policy**

If you believe that this document breaches copyright please contact [librarypure@kcl.ac.uk](mailto:librarypure@kcl.ac.uk) providing details, and we will remove access to the work immediately and investigate your claim.

ORIGINAL ARTICLE



# Predicting the Physiological Effect of Revascularization in Serially Diseased Coronary Arteries

## Clinical Validation of a Novel CT Coronary Angiography–Based Technique

**BACKGROUND:** Fractional flow reserve (FFR) is commonly used to assess the functional significance of coronary artery disease but is theoretically limited in evaluating individual stenoses in serially diseased vessels. We sought to characterize the accuracy of assessing individual stenoses in serial disease using invasive FFR pullback and the noninvasive equivalent, fractional flow reserve by computed tomography (FFR<sub>CT</sub>). We subsequently describe and test the accuracy of a novel noninvasive FFR<sub>CT</sub>-derived percutaneous coronary intervention (PCI) planning tool (FFR<sub>CT-P</sub>) in predicting the true significance of individual stenoses.

**METHODS AND RESULTS:** Patients with angiographic serial coronary artery disease scheduled for PCI were enrolled and underwent prospective coronary CT angiography with conventional FFR<sub>CT</sub>-derived post hoc for each vessel and stenosis (FFR<sub>CT</sub>). Before PCI, the invasive hyperemic pressure-wire pullback was performed to derive the apparent FFR contribution of each stenosis (FFR<sub>pullback</sub>). The true FFR attributable to individual lesions (FFR<sub>true</sub>) was then measured following PCI of one of the lesions. The predictive accuracy of FFR<sub>pullback</sub>, FFR<sub>CT</sub>, and the novel technique (FFR<sub>CT-P</sub>) was then assessed against FFR<sub>true</sub>. From the 24 patients undergoing the protocol, 19 vessels had post hoc FFR<sub>CT</sub> and FFR<sub>CT-P</sub> calculation. When assessing the distal effect of all lesions, FFR<sub>CT</sub> correlated moderately well with invasive FFR ( $R=0.71$ ;  $P<0.001$ ). For lesion-specific assessment, there was significant underestimation of FFR<sub>true</sub> using FFR<sub>pullback</sub> (mean discrepancy,  $0.06\pm 0.05$ ;  $P<0.001$ , representing a 42% error) and conventional trans-lesional FFR<sub>CT</sub> ( $0.05\pm 0.06$ ;  $P<0.001$ , 37% error). Using FFR<sub>CT-P</sub>, stenosis underestimation was significantly reduced to a 7% error ( $0.01\pm 0.05$ ;  $P<0.001$ ).

**CONCLUSIONS:** FFR pullback and conventional FFR<sub>CT</sub> significantly underestimate true stenosis contribution in serial coronary artery disease. A novel noninvasive FFR<sub>CT</sub>-based PCI planner tool more accurately predicts the true FFR contribution of each stenosis in serial coronary artery disease.

**Bhavik N. Modi, MA, MBBS**  
**Sethuraman Sankaran, PhD**  
**Hyun Jin Kim, PhD**  
**Howard Ellis, BSc**  
**Campbell Rogers, MD**  
**Charles A. Taylor, PhD**  
**Ronak Rajani, MBBS, PhD**  
**Divaka Perera, MA, MB Bchir, MD**

**Key Words:** contraindications  
■ coronary angiography ■ coronary artery disease ■ hyperemia  
■ percutaneous coronary intervention

© 2019 The Authors. *Circulation: Cardiovascular Interventions* is published on behalf of the American Heart Association, Inc., by Wolters Kluwer Health, Inc. This is an open access article under the terms of the [Creative Commons Attribution License](https://creativecommons.org/licenses/by/4.0/), which permits use, distribution, and reproduction in any medium, provided that the original work is properly cited.

<https://www.ahajournals.org/journal/circinterventions>

## WHAT IS KNOWN

- Fractional flow reserve (FFR) is commonly used to assess the functional significance of coronary artery disease with noninvasive estimation using FFR by computed tomography (FFR<sub>CT</sub>) growing in popularity.
- Estimating the physiological significance of individual stenoses in the commonly encountered scenario of serial/diffuse coronary artery disease but is theoretically limited with FFR.

## WHAT THE STUDY ADDS

- This study shows that conventional use of FFR and FFR<sub>CT</sub> significantly underestimates true stenosis contribution in serial and diffuse coronary artery disease.
- This study describes a novel noninvasive FFR<sub>CT-P</sub>-based percutaneous coronary intervention planner tool (FFR<sub>CT-P</sub>).
- We show that FFR<sub>CT-P</sub> more accurately predicts the true FFR contribution of each stenosis in serial coronary artery disease, compared with conventional FFR pullback and FFR<sub>CT</sub> outputs.
- The findings of this study would support further large-scale studies examining the validity and applicability of this novel noninvasive percutaneous coronary intervention planning tool.

Coronary computed tomographic angiography (CTA) is now established as a noninvasive test for the detection of significant coronary artery disease (CAD).<sup>1,2</sup> Owing to a relatively low positive predictive value and inability to determine functional significance,<sup>2</sup> CTA has generally been used in patients at a low to intermediate risk with a view to ruling out significant CAD.<sup>3</sup> When coronary atheroma is detected, there is growing evidence that the benefit of revascularization is only derived from targeting myocardial ischemia.<sup>4</sup> Ischemia-guided revascularization has evolved to identifying vessels with functionally significant disease at the time of angiography using indices such as fractional flow reserve (FFR).<sup>5-7</sup> In recent years it has become possible to estimate FFR from standard coronary CTA data sets with FFR by computed tomography (FFR<sub>CT</sub>). Based on computational fluid dynamics (CFD), FFR<sub>CT</sub> has been shown to increase the positive predictive value of coronary CTA and provide clinicians with a noninvasive test to assess coronary anatomy and physiology.<sup>8-10</sup>

The studies validating both invasive FFR and FFR<sub>CT</sub> have largely been in vessels with single epicardial stenoses.<sup>9,11</sup> In reality, CAD is often diffuse in nature with serial stenoses across the length of a vessel. Assessment of the contribution of each stenosis is challenging because physiological interplay affects the

FFR attributable to each stenosis.<sup>12,13</sup> Coronary CTA enables detailed visualization of lesion geometry and a potential to evaluate the true pressure drop across a stenosis by modeling the hemodynamic interplay between serial stenoses.<sup>13</sup> FFR<sub>CT</sub>, therefore, offers the potential to predict the functional significance of individual stenoses within a serially/diffusely diseased vessel, and therefore, to predict the residual functional disease burden following PCI.

In this study, we describe a novel noninvasive FFR<sub>CT</sub>-derived PCI planning tool (FFR<sub>CT-P</sub>), which models physiological interplay between stenoses. This tool is based on a reduced order model informed by 3-dimensional simulations of blood flow to estimate post-PCI pressure loss. In this study we aimed to: (1) characterize the accuracy of estimating individual stenosis significance in serially diseased vessels using invasive FFR pullback and conventional FFR<sub>CT</sub> outputs (usually presented as a color contour map of FFR change down a vessel) and (2) validate the novel noninvasive FFR<sub>CT-P</sub> in a clinical cohort of patients with serial disease, with the aim of comparing the accuracy to estimations made from conventional FFR pullback and FFR<sub>CT</sub>.

## METHODS

The data that support the findings of this study are available from the corresponding author on reasonable request.

### Study Population

All patients recruited to the study gave informed consent. Patients had presented with symptoms of stable angina and had  $\geq 2$  stenoses on an invasive coronary angiogram ( $>30\%$  diameter stenosis by quantified coronary angiography, regardless of whether the stenosis represented a diffuse segment of disease or whether the stenosis was focal). Patients were only eligible if the segments of disease were separated by a normal segment of at least 10 mm, if it were felt feasible to treat each lesion independently by PCI. Exclusion criteria were age  $<18$  years, pregnancy, estimated glomerular filtration rate  $<30$ , previous coronary artery bypass grafting, and contraindications to FFR assessment or CTA. Cardiac catheterization was performed within 4 weeks of the prior CTA scan. The study protocol was approved by the United Kingdom Health Research Authority and local research ethics committee (15/LO/2011).

### CT Protocol

All patients underwent coronary CT angiography using a  $2 \times 192$ -slice dual source CT scanner (Somatom Force, Siemens Medical Solutions, Forchheim), Germany. Eight hundred microgram of sublingual glyceryl trinitrate was administered to all patients along with intravenous metoprolol to achieve a heart rate of  $<65$  bpm in sinus rhythm and  $<100$  bpm in atrial fibrillation. A total of 85 mL intravenous contrast (Omnipaque, GE Healthcare, Princeton, NJ) was injected at 5.5 mL/s by a power injector into the

antecubital vein. Descending aorta contrast triggered, prospective ECG gated scanning with adaptive padding was then performed in a single breath-hold technique after a 10 to 12-second delay. The scanning parameters included a heart rate dependent pitch of 0.2 to 0.45 and a gantry rotation time of 250 ms. The tube voltage was selected semi-automatically, and automated exposure control was used for the tube current. Image slices were reconstructed using a medium sharp kernel (Bv40), using model-based iterative reconstruction strength level 3 (ADMIRE; Siemens Medical Solutions, Forchheim, Germany).

## FFR<sub>CT</sub> Protocol

FFR<sub>CT</sub> analysis was performed by HeartFlow, who were blinded to the invasive angiographic and physiological data. FFR<sub>CT</sub> data were derived post hoc from the CTA data set using methodology that has been previously described.<sup>9,14</sup> In summary, FFR<sub>CT</sub> technology involves extraction of a patient-specific geometric model of the coronary arteries from CTA data. Subsequently, this is combined with population-derived physiological models and CFD techniques to solve the governing equations of blood flow velocity and pressure under simulated hyperemic conditions.<sup>14</sup> FFR<sub>CT</sub> physiological models are based on 3 core scientific principles: an allometric scaling law relating coronary flow to myocardial mass and vessel lumen volume, the principle of flow regulation of vessel size, and an assumption of the predictable reduction of microvascular resistance with maximal hyperemia.<sup>15</sup>

In this study, HeartFlow FFR<sub>CT</sub> v2.7 was used. This software runs on the Amazon Web Services cloud and combines deep-learning artificial intelligence methods<sup>16</sup> to create physiological models that incorporate vessel lumen volume and myocardial mass data.<sup>15</sup> Normal HeartFlow FFR<sub>CT</sub> outputs involve a color-coded chart of continuous FFR<sub>CT</sub> values computed along each vessel. The apparent change in these discrete values across each stenosis within the serially diseased vessel was used to define the attributable FFR<sub>CT</sub> for each stenosis within the serially diseased vessel, using conventional FFR<sub>CT</sub> methods without the planning tool.

## Estimation of FFR<sub>CT</sub> Post-Stenting

To enable the fast recalculation of FFR<sub>CT</sub> for different planning configurations of PCI, an accelerated method for updating FFR<sub>CT</sub> was used (based on a reduced order model derived from CFD simulations). Without compromising on the accuracy of FFR<sub>CT</sub>, this approach is able to update FFR<sub>CT</sub> solutions in real-time in response to changes in lumen geometry. We ensured accuracy was not compromised by comparing the performance of FFR<sub>CT-P</sub> against full conventional FFR<sub>CT</sub> 3D simulations performed on the same models (N=80) and observed that the accuracy was statistically equivalent to that of FFR<sub>CT</sub> (*P* value for equivalence based on 2 one-sided *t* test=0.01). Initially, idealized vessel lumen radii are calculated by first evaluating percent diameter stenosis and subsequently calculating the radius at which there would be no lumen narrowing (ie, to achieve a percent stenosis of zero). Following this, a patient-specific idealized model is constructed using the idealized lumen radii. Finally, a CFD-derived reduced order model is used to calculate the updated FFR<sub>CT</sub> values.

This method involves CFD-derived reduced order model based on a flow-dependent resistance model for the epicardial arteries,  $R=R_{in}+R_{sl}Q$ , where  $R_{in}$  and  $R_{sl}$  are the intercept and slope of the resistance-flow relationship,  $Q$  is the flowrate and

$$R = \frac{\Delta P}{Q} \quad R = \Delta P Q \text{ is the resistance posed by the epicardial vessel}$$

to blood flow. Since these quantities also depend on the epicardial geometry, 2 different flowrates are used to calculate  $R_{in}$  and  $R_{sl}$ . In each of the original and idealized geometries, 2 different boundary conditions, the first being hyperemia as described in the previous section and the second being a 40% lower resistance, are applied. If the flowrates achieved are  $Q$  and  $Q^*$ , and the corresponding resistances calculated from CFD simulations are  $R$  and  $R^*$  then:

$$R_{in} = \frac{(R^*Q - Q^*R)}{(Q - Q^*)} \quad \text{and} \quad R_{sl} = \frac{R^* - R}{Q^* - Q}$$

If the flow difference achieved,  $Q^*-Q$ , is too low, then the intercept and slope are replaced with a 1D CFD model parameterized by lumen area ( $A$ ), viscosity ( $\mu$ ), density ( $\rho$ ), as

$$R_{in} = \frac{8\mu L \pi}{A^2} \quad \text{and} \quad R_{sl} = \frac{\rho L d A}{A^3 dz}$$


These resistances are applied on the updated lumen geometry (where lumen radii in the stented region are replaced by their idealized values), to solve for flow rates, pressures, and FFR<sub>CT</sub>. For the purposes of this study, FFR<sub>CT-P</sub> of each stenosis was derived following the retrospective application of these calculations to CTA images, blinded to invasive FFR values but with knowledge of stent size and position. Figure 1 illustrates the use of this FFR<sub>CT</sub> planner tool in action.

## Cardiac Catheterization Protocol

Angiography was performed via the right radial artery using 6Fr catheters. Before catheterization, all patients received 300 mg of aspirin, 600 mg clopidogrel, and benzodiazepine sedation before local anesthetic was administered. Following arterial puncture, patients received 500 to 1000  $\mu$ g isosorbide dinitrate into the radial artery before cardiac catheters were advanced and a further intracoronary bolus before the acquisition of standard diagnostic images.

## Invasive Pressure-Wire Data Protocol

Before insertion, the pressure-wire was zeroed outside of the body, against a fluid-filled guiding catheter pressure-transducer positioned at the level of the right atrium. After insertion, the pressure sensor was normalized to aortic pressure at the coronary ostium, with the guide disengaged where necessary. The pressure wire tip was delivered to the distal part of the serially-diseased vessel, beyond the distal stenosis (far enough to minimize the effect of post-stenotic turbulent flow), with wire position documented fluoroscopically. An IV adenosine infusion was administered at a dose 140  $\mu$ g  $\text{kg}^{-1} \text{min}^{-1}$  via an antecubital vein. FFR was defined as the lowest Pd/Pa ratio averaged over 5 cardiac cycles following the onset of adenosine.<sup>17</sup> Following documentation of FFR, the pressure-wire was pulled back to the guide catheter during continuous adenosine infusion at a constant

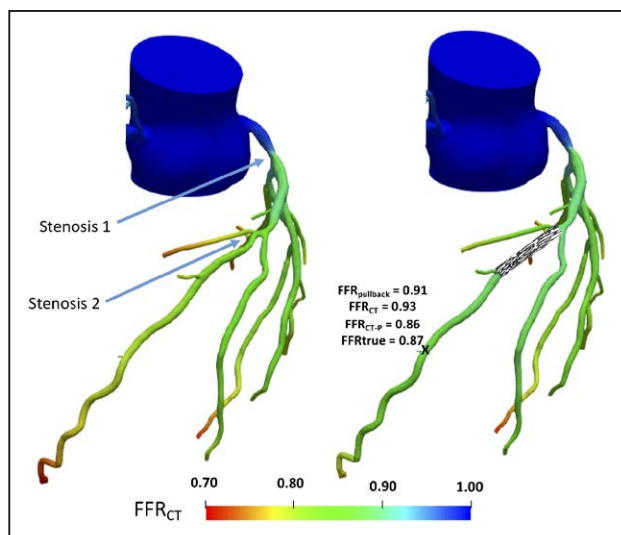

**Figure 1. Example case showing color contour map of fractional flow reserve (FFR) change in a serially diseased vessel with improvement in estimation of true stenosis significance with interactive planner tool.** **Left,** Example of conventional FFR by computed tomography (FFR<sub>CT</sub>) output for a serially diseased left anterior descending artery (serial stenoses labeled) before simulated percutaneous coronary intervention (PCI). The FFR<sub>CT</sub> value between and distal to stenoses is suggested to be 0.93 and 0.80, respectively. **Right,** Results of true measured FFR at point X after PCI of stenosis 2, comparing favorably with FFR<sub>CT</sub>-derived PCI planning tool (FFR<sub>CT-p</sub>), following application of novel planner tool. Using conventional FFR<sub>CT</sub> and FFR<sub>pullback</sub>, the underestimation would have been more significant (0.93 and 0.91, respectively).

speed (roughly 1 mm/s). This was done through the whole of the vessel, regardless of what the operator felt was a significant stenosis.

The apparent change in hyperemic pressure gradient across each stenosis following pressure-wire pullback within the serially diseased vessel was noted with the attributable FFR termed FFR<sub>pullback</sub>. PCI was then performed, with the choice of stenosis treated at the discretion of the operator using their conventional practice. Following re-calibration, pressure-wire pullback was then repeated (ensuring the stented segment no longer poses any pressure gradient). The subsequent true change in hyperemic pressure gradient across the remaining stenosis in isolation was noted with the stenosis-attributable FFR termed FFR<sub>true</sub> (ie, FFR in the vessel following PCI of the accompanying serial stenosis). The difference between FFR<sub>true</sub> and FFR<sub>pullback</sub> was indicative of the degree of stenosis underestimation in serial CAD. The relationship between the extent of stenosis underestimation and total vessel FFR (the cumulative FFR in the vessel before PCI when both stenoses were present) was also assessed for each invasive and noninvasive index.

## Statistical Analysis

SPSS Version 23 (IBM Corp, Armonk, New York) and Prism Graphpad 5.0 (GraphPad Software Inc, CA) were used for all analyses. Normality was assessed using a visual assessment of histograms and Q-Q plots. Continuous data are expressed as mean±SD and compared using paired *t* tests. A 2-tailed test of significance was performed for all analyses with *P*<0.05 being considered statistically significant. Correlations were assessed using Pearson correlation coefficients (*R*).

Bland-Altman analysis was used to compare the differences between estimated and true value across the range of measurements.

In addition, methods were compared in estimating the true post-PCI change in FFR across a stenosis. This was done by calculating the mean relative error (essentially the error as a proportion of the true FFR gradient across the lesion). This mean error is essentially calculated by evaluating the absolute difference between the true FFR gradient and the predicted FFR gradient (either using conventional FFR<sub>CT</sub> or the novel FFR<sub>CT-p</sub>) and dividing this by the true FFR gradient across the stenosis in question.

## RESULTS


Twenty-seven patients had prospective CT coronary angiography that demonstrated serial CAD in 30 vessels. Of these, 5 patients (6 vessels) were excluded as satisfactory catheter laboratory data could not be obtained (reasons were: stenosis deemed too severe to make pressure-wire measurements, vessel tortuosity making it difficult to pass pressure-wire, and an adverse reaction to adenosine). Of the remaining 24 vessels, 19 (79%) had satisfactory computation of FFR<sub>CT</sub> along the vessel (Figure 2 for study flow chart). Three patients were excluded because of proximal stented segments and 2 owing to CTA motion artifacts that precluded post hoc FFR<sub>CT</sub> computation.

Patients included, in the final analysis, had a median age of 64.7 years (89% male). The Table summarizes the patient demographics and details of the serially diseased vessels. FFR of these vessels was 0.67±0.16. Total vessel FFR<sub>CT</sub> of these vessels was 0.68±0.18. The Invasive total vessel FFR showed reasonable agreement with total vessel FFR<sub>CT</sub>, in line with previous studies<sup>8,9</sup> (Pearson's *R*=0.71). Scatterplot and a Bland-Altman plot comparing invasive total vessel FFR with total vessel FFR<sub>CT</sub> are shown in Figure 3.

With FFR pullback, significant underestimation of stenosis contribution occurred, regardless of whether the proximal or distal lesion was considered, with a mean difference between FFR<sub>pullback</sub> and FFR<sub>true</sub> of 0.06±0.05 (*P*<0.001). This corresponded to a mean relative error of 42%. For conventional FFR<sub>CT</sub> outputs along the course of vessels, similar significant underestimation of stenosis contribution occurred, with a mean difference between FFR<sub>CT</sub> and FFR<sub>true</sub> of 0.05±0.06 (*P*<0.001), giving a mean relative error of 37%.

## Estimating True Stenosis Significance With Interactive Planner Tool

Using the newly developed interactive FFR<sub>CT</sub> PCI planning tool, we were able to estimate the FFR in the vessel FFR<sub>CT-p</sub> following PCI of one of the 2 serial stenoses (example case shown in Figure 1). Optimal PCI was

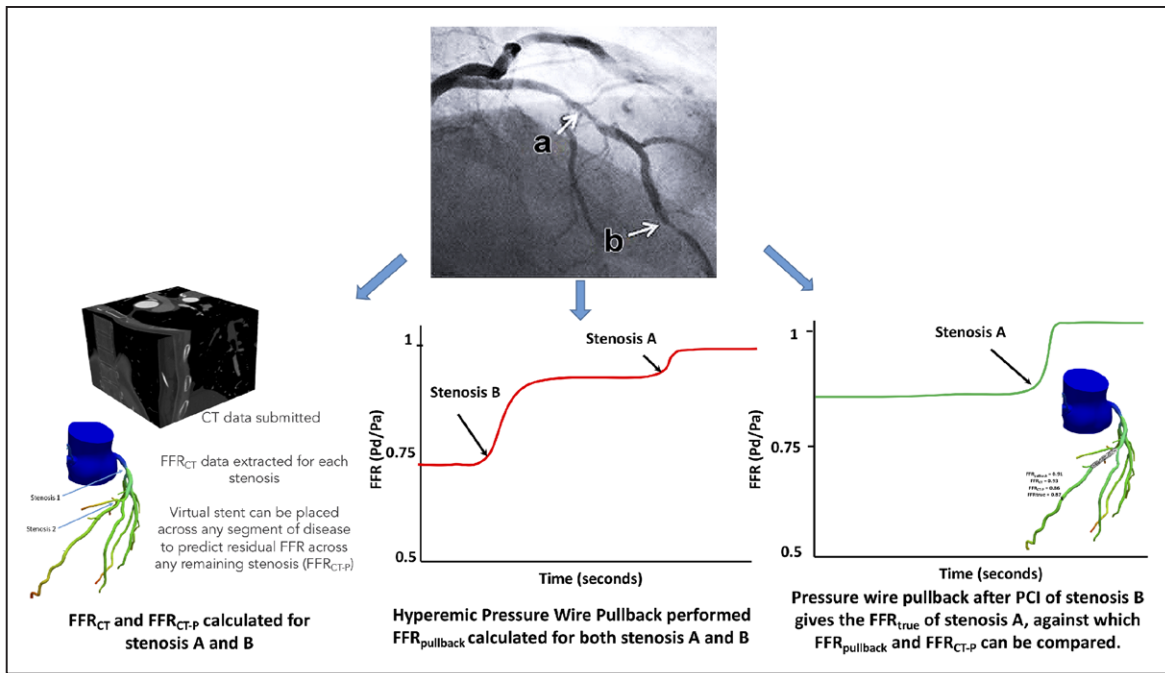

**Figure 2.** Study flow diagram.

The Figure shows how fractional flow reserve by computed tomography (FFR<sub>CT</sub>)-derived percutaneous coronary intervention (PCI) planning tool (FFR<sub>CT-P</sub>) and FFR<sub>pullback</sub> were calculated and subsequently compared with FFR<sub>true</sub>.

performed in 13 patients, with pressure wire pullback performed following PCI to ensure no residual lumen narrowing and pressure drop across the stented portion before assessing FFR<sub>true</sub> (Figure 2 study flow chart).

Use of FFR<sub>CT-P</sub> resulted in a significant improvement in the correlation between the predicted FFR<sub>CT</sub> and FFR<sub>true</sub> following PCI of one of the 2 serial stenoses (R=0.44 with conventional FFR<sub>CT</sub>, improving significantly to R=0.75 with FFR<sub>CT-P</sub>; Figure 4). Whilst there was good direct correlation of per-stenosis FFR<sub>CT-P</sub> to FFR<sub>true</sub> (Pearson correlation coefficient 0.75, P=0.001; Figure 4), in a few cases there was significant over/under-estimation, particularly when the baseline total vessel FFR was <0.7). Figure 4 also illustrates the performance using FFR<sub>pullback</sub>. FFR<sub>CT-P</sub> has a better correlation coefficient and a more linear fit to the data compared to FFR<sub>CT</sub> or FFR<sub>pullback</sub>.

By applying the interactive planner tool on a geometry matching the stent location in the subsequent PCI, the absolute value of underestimation fell to 0.01±0.05, which corresponded to a mean proportional error of 7% (Figure 5). The equation performed equally well in the 2 cases where one of the 2 stenoses was diffuse (stenosis measured >30 mm in length by quantified coronary angiography).

## DISCUSSION

In this study, we have shown that (1) using an unadjusted trans-lesional gradient from conventional FFR<sub>CT</sub> outputs leads to significant underestimation of stenosis contribution in serially diseased vessels, similar


to invasive FFR pullback methods and (2) applying a novel interactive PCI planning tool (FFR<sub>CT-P</sub>), results in a significant improvement in the accuracy of predicting the residual true FFR contribution of stenoses following treatment of accompanying serial stenoses. To our knowledge, this is the first description and validation of this novel noninvasive method to predict the hemodynamic outcome of a PCI procedure.

Serial and diffuse CAD is common, particularly within aging and diabetic populations, with estimates of 25% to 40% prevalence in all patients presenting for angiography.<sup>18,19</sup> There are, however, several well-established limitations of physiological assessment of serial CAD. A simple explanation for this

**Table.** Summary of Patient Demographics and Lesion Characteristics

Age, years	64.7 ±12.0
Male	17 (89%)
Hypertension	12 (63%)
Diabetes mellitus	6 (32%)
Smoker	5 (26%)
Hyperlipidemia	15 (79%)
Previous PCI	6 (32%)
Lesion severity (by QCA)	58.9%
Lesion length, mm	11.3
Lesion separation, mm	18.6

Summary of patient demographics and lesion characteristics for 24 patients recruited to the study. Data presented as mean values±SD with percentage prevalence where relevant. PCI indicates percutaneous coronary intervention; and QCA; quantified coronary angiography.

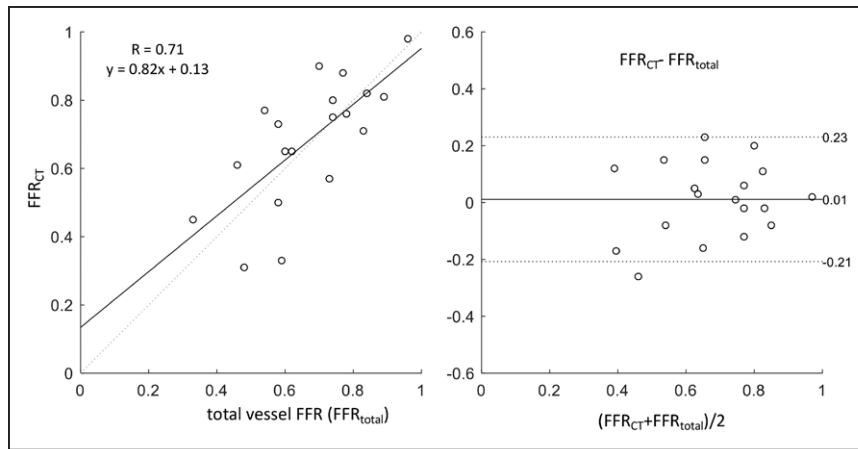


**Figure 3. Scatter and Bland-Altman plots comparing fractional flow reserve by computed tomography ( $FFR_{CT}$ ) against invasive FFR before percutaneous coronary intervention (PCI).**

**Left**, Scatterplot comparing  $FFR_{CT}$  against invasively measured FFR before PCI. Solid lines represent the best linear fit to the data, and dotted lines represents the line of identity ( $x=y$ ). **Right**, Bland-Altman plot comparing the differences between total vessel  $FFR_{CT}$  and total vessel FFR. Solid line represents the mean difference, and dotted lines correspond to the 95% CIs.

is that a stenosis provides resistance to blood flow, manifesting as a post-stenotic drop in pressure that is magnified in hyperemic conditions to give the true FFR when present in isolation. When another stenosis or diffusely-diseased segment, maximal hyperemia (and, therefore, measurement of the true FFR resulting from the stenoses) is not possible because of the additional resistance to flow, with the situation further complicated by flow turbulence when stenoses are particularly severe, close together and nonconcentric.<sup>13,20</sup> The techniques previously described to overcome these limitations have been complex; requiring measurement of coronary wedge pressure<sup>12</sup> or the presence of a disease-free daughter branch when serial disease involves the left main coronary artery.<sup>21</sup> Although it has been suggested that resting indices (eg, iFR pullback) might result in smaller absolute errors than FFR


in this setting,<sup>22</sup> this is likely to be a reflection of the different operating range of resting indices, which are also prone to significant error.

At present, conventional  $FFR_{CT}$  outputs are presented as color-coded maps of coronary arteries showing how  $FFR_{CT}$  values change down the vessel. These color-coded gradients of  $FFR_{CT}$  are designed to mirror the changes in measured FFR one would expect with a hyperemic pressure-wire pullback within the catheter laboratory. In keeping with this, our results show that unadjusted trans-lesional gradients from these conventional  $FFR_{CT}$  outputs show a similarly significant degree of stenosis underestimation in serially diseased vessels, as is the case with invasive FFR pullback. Given that the physiological interplay largely depends on lesion geometry, which in turn can be well characterized by CTA techniques, a  $FFR_{CT}$ -based technique would be expected to

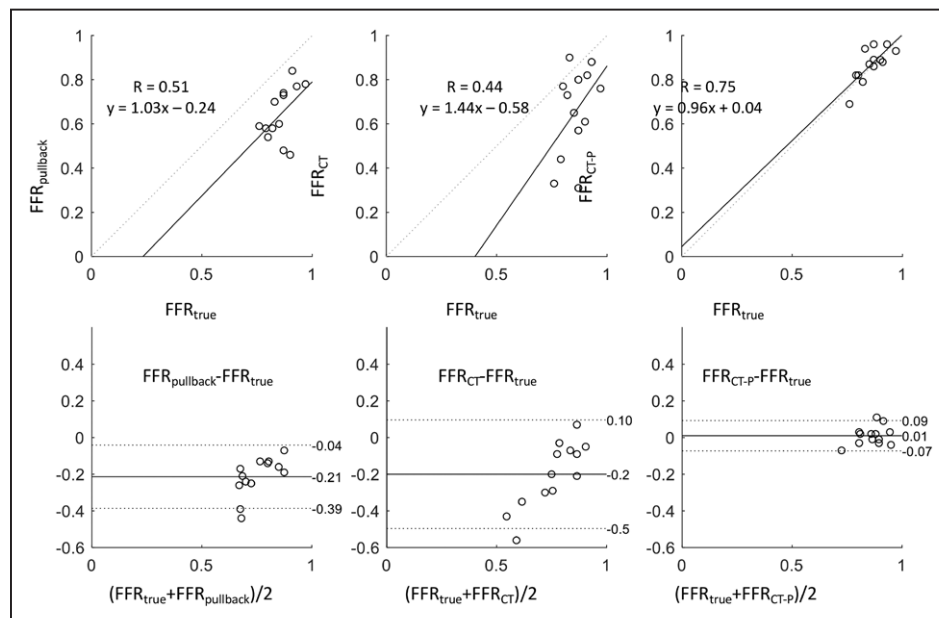

**Figure 4. Scatter and Bland-Altman plots demonstrating how planner tool improves estimation of  $FFR_{true}$ .**

**Top**, Scatterplots comparing the (left to right)  $FFR_{pullback}$ ,  $FFR$  by computed tomography ( $FFR_{CT}$ ), and  $FFR_{CT}$ -derived percutaneous coronary intervention (PCI) planning tool ( $FFR_{CT-P}$ ) against true FFR. Solid lines represent the best linear fit to the data and dotted lines represents the line of identity ( $x=y$ ). **Bottom**, Bland-Altman plot comparing the differences between  $FFR_{true}$  and  $FFR_{pullback}$ ,  $FFR_{CT}$ , and  $FFR_{CT-P}$  (left to right). Solid line represents the mean difference, and dotted lines correspond to the 95% CIs. FFR indicates fractional flow reserve.

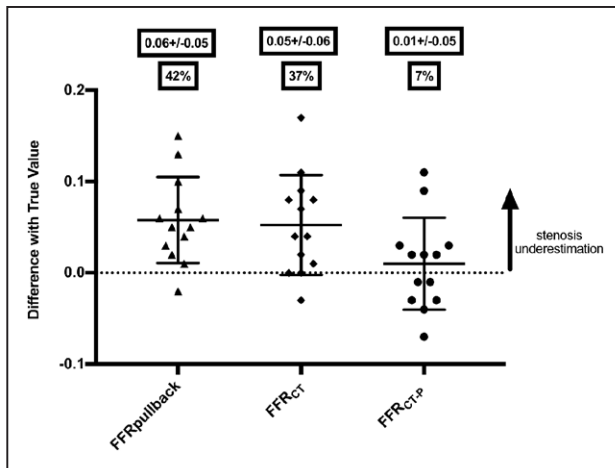

**Figure 5. Categorical scatter plot comparing errors in estimating true stenosis significance with different methods.**

Categorical scatter plot comparing errors in estimating true stenosis significance (mean error $\pm$ SD) with invasive FFR<sub>pullback</sub> vs conventional FFR by computed tomography (FFR<sub>CT</sub>) vs results from FFR<sub>CT</sub> with the percutaneous coronary intervention (PCI) planning tool (FFR<sub>CT-P</sub>). Also shown are percentage errors for each physiological tool as a proportion of the true FFR change, derived following isolation of a stenosis by PCI of an accompanying tandem stenosis. FFR indicates fractional flow reserve.

have greater potential at predicting the true physiological contribution of an individual stenosis, with the added appeal of being a noninvasive technique. Based on this, the FFR<sub>CT-P</sub> has been developed to allow real-time recalculation of residual FFR after simulating PCI, with the operator able to choose simulated stent position and length.

Despite the large and significant reduction in mean error using the novel FFR<sub>CT</sub> method (FFR<sub>CT-P</sub>), the variance of the error because of serial disease is still appreciable (SD  $\pm$  0.05), particularly when the cumulative burden of disease in the vessel is high (ie, total FFR low). These findings are consistent with previous meta-analyses of FFR<sub>CT</sub> diagnostic performance that have shown reduced accuracy with more severe stenoses.<sup>23</sup> This may be as a result of limited CT visualization of stenosis geometry when stenoses are severe but also variability in microvascular function which is difficult to predict from a noninvasive functional-anatomic test. In addition, the geometry of the untreated lesion can change post-PCI because of a higher operating pressure and can lead to unaccounted changes in FFR<sub>CT</sub>.<sup>21</sup> There are several additional issues when using FFR<sub>CT</sub> in planning intervention that may limit the utility of such a noninvasive tool: Firstly, there is a need to have an appropriate CT scan within a few weeks of the planned PCI. Secondly, not all prospectively acquired CT scans are of adequate quality for FFR<sub>CT</sub> computation. Within our study, around 20% of cases could not have post hoc FFR<sub>CT</sub> computation because of issues such as phase misalignment. This was a rate similar to the NXT trial where 13% of CT scans were unsuitable for analysis owing to inadequate image quality issues such as phase misalignment, stent-related artifacts, and blooming.<sup>9</sup>

Despite these factors, in patients that are able to have an adequate quality prospective CT coronary angiogram before planned PCI, FFR<sub>CT-P</sub> still represents a significant improvement to current methods of physiologically assessing serial CAD. Furthermore, it has the potential to complement contemporary methods of planning PCI, particularly in patients with serial/diffuse CAD, without requiring the invasive positioning of a coronary guidewire. Further multi-center data will be needed to evaluate this tool and its impact of clinical decision-making.

## Limitations

1. The study is limited by its relatively small sample size and, therefore, the results are primarily hypothesis generating and merit further examination in a larger population derived from a multicenter setting.
2. In addition, FFR<sub>CT</sub> has not been validated for patients with previous coronary artery bypass, previous stenting within the same vessel, or significantly abnormal left ventricular function, and therefore, by extension we excluded these patients, and we cannot extrapolate the results from the FFR<sub>CT</sub> PCI planning tool to those patient groups.

## Conclusions

FFR<sub>CT</sub> provides a comparable estimation of FFR values obtained from routine invasive pressure-wire pullback along a vessel and is prone to a similar degree of physiological underestimation in serial CAD. In this study, we provide validation for a novel noninvasive FFR<sub>CT-P</sub> and show it to significantly reduce the error of contemporary methods in estimating true stenosis contribution within serially diseased vessels following PCI of an accompanying stenosis.

## ARTICLE INFORMATION

Received October 29, 2018; accepted December 19, 2018.

### Correspondence

Divaka Perera, MA MBBChir MD, Cardiovascular Division, Rayne Institute, St. Thomas' Hospital, London, SE1 7EH. Email [divaka.perera@kcl.ac.uk](mailto:divaka.perera@kcl.ac.uk)

### Affiliations

NIHR Biomedical Research Centre and British Heart Foundation Centre of Excellence, School of Cardiovascular Medicine and Sciences, King's College London (B.N.M., H.E., R.R., D.P.) and HeartFlow Inc, Redwood City, California (S.S., H.J.K., C.R., C.A.T.).

### Acknowledgments

David Lesage (employee at HeartFlow Inc) helped generate the FFR<sub>CT</sub> patient-specific idealized lumen radii models. We acknowledge the ongoing support of the British Heart Foundation in supporting cardiovascular research in our institution and the United Kingdom as a whole.



## Sources of Funding

B. Modi is funded by a British Heart Foundation Clinical Research Training Fellowship (FS/15/78/31678) and D. Perera is supported by the United Kingdom National Institutes for Health Research via the Biomedical Research Centre award to King's College London.

## Disclosures

Heart Flow Inc have borne the costs of post-processing CTA data. S. Sankaran, H.J. Kim, C. Rogers, and C.A. Taylor are Heart Flow Inc employees.

## REFERENCES

- Miller JM, Rochitte CE, Dewey M, Arbab-Zadeh A, Niinuma H, Gottlieb I, Paul N, Clouse ME, Shapiro EP, Hoe J, Lardo AC, Bush DE, de Roos A, Cox C, Brinker J, Lima JA. Diagnostic performance of coronary angiography by 64-row CT. *N Engl J Med*. 2008;359:2324–2336. doi: 10.1056/NEJMoa0806576
- Budoff MJ, Dowe D, Jollis JG, Gitter M, Sutherland J, Halamert E, Scherer M, Bellinger R, Martin A, Benton R, Delago A, Min JK. Diagnostic performance of 64-multidetector row coronary computed tomographic angiography for evaluation of coronary artery stenosis in individuals without known coronary artery disease: results from the prospective multicenter ACCURACY (Assessment by Coronary Computed Tomographic Angiography of Individuals Undergoing Invasive Coronary Angiography) trial. *J Am Coll Cardiol*. 2008;52:1724–1732. doi: 10.1016/j.jacc.2008.07.031
- Taylor AJ, Cerqueira M, Hodgson JM, Mark D, Min J, O'Gara P, Rubin GD; American College of Cardiology Foundation Appropriate Use Criteria Task Force; Society of Cardiovascular Computed Tomography; American College of Radiology; American Heart Association; American Society of Echocardiography; American Society of Nuclear Cardiology; North American Society for Cardiovascular Imaging; Society for Cardiovascular Angiography and Interventions; Society for Cardiovascular Magnetic Resonance. ACCF/SCCT/ACR/AHA/ASE/ASNC/NASCI/SCAI/SCMR 2010 Appropriate Use Criteria for Cardiac Computed Tomography. A Report of the American College of Cardiology Foundation Appropriate Use Criteria Task Force, the Society of Cardiovascular Computed Tomography, the American College of Radiology, the American Heart Association, the American Society of Echocardiography, the American Society of Nuclear Cardiology, the North American Society for Cardiovascular Imaging, the Society for Cardiovascular Angiography and Interventions, and the Society for Cardiovascular Magnetic Resonance. *Circulation*. 2010;122:e525–e555. doi: 10.1161/CIR.0b013e3181fae66
- Hachamovitch R, Hayes SW, Friedman JD, Cohen I, Berman DS. Comparison of the short-term survival benefit associated with revascularization compared with medical therapy in patients with no prior coronary artery disease undergoing stress myocardial perfusion single photon emission computed tomography. *Circulation*. 2003;107:2900–2907. doi: 10.1161/01.CIR.0000072790.23090.41
- Pijls NH, De Bruyne B, Peels K, Van Der Voort PH, Bonnier HJ, Bartunek J, Koolen JJ, Koolen JJ. Measurement of fractional flow reserve to assess the functional severity of coronary-artery stenoses. *N Engl J Med*. 1996;334:1703–1708. doi: 10.1056/NEJM199606273342604
- De Bruyne B, Pijls NHJ, Kalesan B, Barbato E, Tonino PAL, Piroth Z, Jagic N, Möbius-Winkler S, Rioufol G, Witt N, Kala P, MacCarthy P, Engström T, Oldroyd KG, Mavromatis K, Manoharan G, Verlee P, Frobert O, Curzen N, Johnson JB, Jüni P, Fearon WF. Fractional flow reserve–guided PCI versus medical therapy in stable coronary disease. *N Engl J Med*. 2012;367:991–1001. doi: 10.1056/NEJMoa1205361
- Tonino PA, De Bruyne B, Pijls NH, Siebert U, Ikeno F, van't Veer M, Klauss V, Manoharan G, Engström T, Oldroyd KG, Ver Lee PN, MacCarthy PA, Fearon WF; FAME Study Investigators. Fractional flow reserve versus angiography for guiding percutaneous coronary intervention. *N Engl J Med*. 2009;360:213–224. doi: 10.1056/NEJMoa0807611
- Douglas PS, Pontone G, Hlatky MA, Patel MR, Norgaard BL, Byrne RA, Curzen N, Purcell I, Gutberlet M, Rioufol G, Hink U, Schuchlenz HW, Feuchtnner G, Gilard M, Andreini D, Jensen JM, Hadamitzky M, Chiswell K, Cyr D, Wilk A, Wang F, Rogers C, De Bruyne B; PLATFORM Investigators. Clinical outcomes of fractional flow reserve by computed tomographic angiography-guided diagnostic strategies vs. usual care in patients with suspected coronary artery disease: the prospective longitudinal trial of FFR(CT): outcome and resource impacts study. *Eur Heart J*. 2015;36:3359–3367. doi: 10.1093/eurheartj/ehv444
- Nørgaard BL, Leipsic J, Gaur S, Senviratne S, Ko BS, Ito H, Jensen JM, Mauri L, De Bruyne B, Bezerra H, Osawa K, Marwan M, Naber C, Erglis A, Park SJ, Christiansen EH, Kalltoft A, Lassen JF, Bøtker HE, Achenbach S; NXT Trial Study Group. Diagnostic performance of noninvasive fractional flow reserve derived from coronary computed tomography angiography in suspected coronary artery disease: the NXT trial (Analysis of Coronary Blood Flow Using CT Angiography: Next Steps). *J Am Coll Cardiol*. 2014;63:1145–1155. doi: 10.1016/j.jacc.2013.11.043
- Koo BK, Erglis A, Doh JH, Daniels DV, Jegere S, Kim HS, Dunning A, DeFrance T, Lansky A, Leipsic J, Min JK. Diagnosis of ischemia-causing coronary stenoses by noninvasive fractional flow reserve computed from coronary computed tomographic angiograms. Results from the prospective multicenter DISCOVER-FLOW (Diagnosis of Ischemia-Causing Stenoses Obtained Via Noninvasive Fractional Flow Reserve) study. *J Am Coll Cardiol*. 2011;58:1989–1997. doi: 10.1016/j.jacc.2011.06.066
- De Bruyne B, Pijls NH, Kalesan B, Barbato E, Tonino PA, Piroth Z, Jagic N, Möbius-Winkler S, Möbius-Winkler S, Rioufol G, Witt N, Kala P, MacCarthy P, Engström T, Oldroyd KG, Mavromatis K, Manoharan G, Verlee P, Frobert O, Curzen N, Johnson JB, Jüni P, Fearon WF; FAME 2 Trial Investigators. Fractional flow reserve–guided PCI versus medical therapy in stable coronary disease. *N Engl J Med*. 2012;367:991–1001. doi: 10.1056/NEJMoa1205361
- Pijls NH, De Bruyne B, Bech GJ, Liistro F, Heyndrickx GR, Bonnier HJ, Koolen JJ. Coronary pressure measurement to assess the hemodynamic significance of serial stenoses within one coronary artery: validation in humans. *Circulation*. 2000;102:2371–2377.
- Modi BN, De Silva K, Rajani R, Curzen N, Perera D. Physiology-guided management of serial coronary artery disease: a review. *JAMA Cardiol*. 2018;3:432–438. doi: 10.1001/jamacardio.2018.0236
- Taylor CA, Fonte TA, Min JK. Computational fluid dynamics applied to cardiac computed tomography for noninvasive quantification of fractional flow reserve: scientific basis. *J Am Coll Cardiol*. 2013;61:2233–2241. doi: 10.1016/j.jacc.2012.11.083
- Taylor CA, Gaur S, Leipsic J, Achenbach S, Berman DS, Jensen JM, Dey D, Bøtker HE, Kim HJ, Khem S, Wilk A, Zarins CK, Bezerra H, Lesser J, Ko B, Narula J, Ahmadi A, Øvrehus KA, St Goar F, De Bruyne B, Nørgaard BL. Effect of the ratio of coronary arterial lumen volume to left ventricle myocardial mass derived from coronary CT angiography on fractional flow reserve. *J Cardiovasc Comput Tomogr*. 2017;11:429–436. doi: 10.1016/j.jcct.2017.08.001
- LeCun Y, Bengio Y, Hinton G. Deep learning. *Nature*. 2015;521:436–444. doi: 10.1038/nature14539
- Johnson NP, Johnson DT, Kirkeide RL, Berry C, De Bruyne B, Fearon WF, Oldroyd KG, Pijls NHJ, Gould KL. Repeatability of fractional flow reserve despite variations in systemic and coronary hemodynamics. *JACC Cardiovasc Interv*. 2015;8:1018–1027. doi: 10.1016/j.jcin.2015.01.039
- Dortimer AC, Shenoy PN, Shiroff RA, Leaman DM, Babb JD, Liedtke AJ, Zelis R. Diffuse coronary artery disease in diabetic patients: fact or fiction? *Circulation*. 1978;57:133–136.
- Di Sciascio G, Patti G, Nasso G, Manzoli A, D'Ambrosio A, Abbate A. Early and long-term results of stenting of diffuse coronary artery disease. *Am J Cardiol*. 2000;86:1166–1170.
- Kern MJ, Seto AH. A perspective on physiologic assessment of coronary stenoses in series: methods, myths, and best practices? *JAMA Cardiol*. 2018;3:368–370. doi: 10.1001/jamacardio.2018.0239
- Fearon WF, Yong AS, Lenders G, Toth GG, Dao C, Daniels DV, Pijls NHJ, De Bruyne B. The impact of downstream coronary stenosis on fractional flow reserve assessment of intermediate left main coronary artery disease: human validation. *JACC Cardiovasc Interv*. 2015;8:398–403. doi: 10.1016/j.jcin.2014.09.027
- Nijjer SS, Sen S, Petraco R, Escaned J, Echavarría-Pinto M, Broyd C, Al-Lamee R, Foin N, Foale RA, Malik IS, Mikhail GW, Sethi AS, Al-Bustami M, Kaprielian RR, Khan MA, Baker CS, Bellamy MF, Hughes AD, Mayet J, Francis DP, Di Mario C, Davies JE. Pre-angioplasty instantaneous wave-free ratio pullback provides virtual intervention and predicts hemodynamic outcome for serial lesions and diffuse coronary artery disease. *JACC Cardiovasc Interv*. 2014;7:1386–1396. doi: 10.1016/j.jcin.2014.06.015
- Cook CM, Petraco R, Shun-Shin MJ, Ahmad Y, Nijjer S, Al-Lamee R, Kikuta Y, Shiono Y, Mayet J, Francis DP, Sen S, Davies JE. Diagnostic accuracy of computed tomography-derived fractional flow reserve: a systematic review. *JAMA Cardiol*. 2017;2:803–810. doi: 10.1001/jamacardio.2017.1314