



King's Research Portal

DOI:

[10.1016/j.amjcard.2016.03.028](https://doi.org/10.1016/j.amjcard.2016.03.028)

Document Version

Peer reviewed version

[Link to publication record in King's Research Portal](#)

Citation for published version (APA):

Eskandari, M., Aldalati, O., Byrne, J., Dworakowski, R., Wendler, O., Alcock, E., Monaghan, M., & MacCarthy, P. (2016). Zero Contrast Transfemoral Transcatheter Aortic Valve Replacement (TAVR) Using Fluoroscopy-Echocardiography Fusion Imaging. *American Journal of Cardiology*. Advance online publication. <https://doi.org/10.1016/j.amjcard.2016.03.028>

Citing this paper

Please note that where the full-text provided on King's Research Portal is the Author Accepted Manuscript or Post-Print version this may differ from the final Published version. If citing, it is advised that you check and use the publisher's definitive version for pagination, volume/issue, and date of publication details. And where the final published version is provided on the Research Portal, if citing you are again advised to check the publisher's website for any subsequent corrections.

General rights

Copyright and moral rights for the publications made accessible in the Research Portal are retained by the authors and/or other copyright owners and it is a condition of accessing publications that users recognize and abide by the legal requirements associated with these rights.

- Users may download and print one copy of any publication from the Research Portal for the purpose of private study or research.
- You may not further distribute the material or use it for any profit-making activity or commercial gain
- You may freely distribute the URL identifying the publication in the Research Portal

Take down policy

If you believe that this document breaches copyright please contact librarypure@kcl.ac.uk providing details, and we will remove access to the work immediately and investigate your claim.

Accepted Manuscript



Zero Contrast Transfemoral Transcatheter Aortic Valve Replacement (TAVR) Using Fluoroscopy-Echocardiography Fusion Imaging

Mehdi Eskandari, MD, Omar Aldalati, MD, Jonathan Byrne, MBChB, PhD, Rafal Dworakowski, MD, PhD, Olaf Wendler, MD, PhD, Ema Alcock, MBBS, Mark Monaghan, PhD, Philip MacCarthy, BSc MBChB, PhD.

PII: S0002-9149(16)30374-5

DOI: [10.1016/j.amjcard.2016.03.028](https://doi.org/10.1016/j.amjcard.2016.03.028)

Reference: AJC 21769

To appear in: *The American Journal of Cardiology*

Received Date: 7 February 2016

Accepted Date: 14 March 2016

Please cite this article as: Eskandari M, Aldalati O, Byrne J, Dworakowski R, Wendler O, Alcock E, Monaghan M, MacCarthy P, Zero Contrast Transfemoral Transcatheter Aortic Valve Replacement (TAVR) Using Fluoroscopy-Echocardiography Fusion Imaging, *The American Journal of Cardiology* (2016), doi: 10.1016/j.amjcard.2016.03.028.

This is a PDF file of an unedited manuscript that has been accepted for publication. As a service to our customers we are providing this early version of the manuscript. The manuscript will undergo copyediting, typesetting, and review of the resulting proof before it is published in its final form. Please note that during the production process errors may be discovered which could affect the content, and all legal disclaimers that apply to the journal pertain.

Zero Contrast Transfemoral Transcatheter Aortic Valve Replacement (TAVR) Using
Fluoroscopy-Echocardiography Fusion Imaging

Short Title: Zero Contrast TAVR

Mehdi Eskandari, MD, Omar Aldalati MD, Jonathan Byrne, MBChB, PhD, Rafal Dworakowski, MD, PhD, Olaf Wendler, MD, PhD, Ema Alcock, MBBS, Mark Monaghan, PhD, Philip MacCarthy BSc MBChB, PhD.

King's College Hospital, London, UK

Corresponding Author:

Mehdi Eskandari
Suit 6, Golden Jubilee Building
King's College Hospital
Denmark Hill
London
UK, SE59RS

Phone: 00447903798465

Email: Mehdi.Eskandari@nhs.net

Acute kidney injury (AKI) remains a major concern in the field of TAVR and is associated with increased mortality, up to 2-8 fold (1). Although the exact mechanism of post-TAVR AKI is unknown and seems to be multifactorial, contrast has been reported as a contributing factor (2). During TAVR, contrast is used for conventional aortic root angiography, for positioning of the TAVR valve device and assessing the peripheral vasculature. To our knowledge, for the first time we report transfemoral TAVR performed with zero contrast using fluoroscopy and ultrasound guidance. This was done in two patients with symptomatic, severe aortic stenosis and significant chronic kidney disease (stage III) who were deemed high risk for surgical aortic valve replacement after discussion in the multidisciplinary Heart Team meeting.

EchoNavigator system (Phillips Healthcare, Netherland) is a novel imaging technology which allows fusion of real time 2D and 3D echocardiography images on the fluoroscopy screen. It has the ability to identify the optimal perpendicular valve view without use of contrast (Figure 1), can provide a road map to assist crossing of the aortic valve in difficult cases and enables overlay of echocardiographic images on the X-ray screen so that the the soft tissue characterization of echocardiography is combined with excellent device visualization of X-ray to assure precise device deployment. Determining the optimal valve view is a crucial prerequisite for accurate positioning of the bioprosthetic valve to avoid potentially life-threatening complications. Although aortic root angiography is conventionally used to identify the valve view, EchoNavigator can be solely used for this purpose. Moreover, to further minimise exposure to contrast, 3D transesophageal echocardiography (TEE), which is the standard technique in our centre, was used for valve sizing.

Procedures were done under general anesthesia. As per routine practice in our centre, we used a handheld ultrasound device for establishing vascular access in both patients which also

allowed assessment of patency of the femoral arteries at the end of the procedure without the use of contrast.

For the first patient, a 27 mm Lotus valve (Boston Scientific) was positioned under combined fluoroscopy and fusion imaging guidance (Figure 2). Intra procedural 2D colour Doppler assessment of the positioned valve revealed mild to moderate paravalvular aortic regurgitation (AR) resulting from under-expansion of the valve at the site of severely calcified non-coronary cusp. Despite attempts to reposition the valve, the paravalvular AR remained unchanged. Although there is very limited data on post dilatation of the Lotus valve (3), based on previous successful experience in our centre, we decided to post dilate using a 24 mm balloon, which resulted in complete resolution of the paravalvular AR. A 26 mm Sapien 3 (Edwards Lifesciences) valve was used for the second case and deployed under fluoro-echo fusion imaging with no paravalvular AR assessed by TEE at the end of the procedure (Figure 3). A thorough echocardiographic assessment was performed at the end of each procedure to exclude new regional wall motion abnormalities.

Both patients had an excellent post-procedure recovery and were discharged home on day three with no change in renal function, no residual trans-aortic valvular gradient and no paravalvular AR.

Fluoro-echo fusion imaging can be used to minimise the contrast use in patients at high risk of developing AKI. The technique has the potential to be routinely used in performing TAVR with zero contrast. Further studies are required to assess the impact of zero contrast strategy on patients' outcome.

Mehdi Eskandari MD
Omar Aldalati MD
Jonathan Byrne PhD
Rafal Dworakowski MD, PhD

Olaf Wendler, MD, PhD
Ema Alcock, MBBS
Mark Monaghan PhD
Philip MacCarthy PhD

London, United Kingdom

10 February 2016

ACCEPTED MANUSCRIPT

References

1. Najjar M, Salna M, George I. Acute kidney injury after aortic valve replacement: incidence, risk factors and outcomes. *Expert Rev Cardiovasc Ther* 2015;13:301-316.
2. Elhmidi Y, Bleiziffer S, Deutsch MA, Krane M, Mazzitelli D, Lange R, Piazza N. Acute kidney injury after transcatheter aortic valve implantation: incidence, predictors and impact on mortality. *Arch Cardiovasc Dis* 2014;107:133-139.
3. Fuchs F, Tiyerili V, Roell W, Grube E, Werner N, Nickenig G, Sinning JM. Successful post-dilation of a lotus transcatheter aortic valve in a case of prosthesis frame underexpansion due to leaflet calcification. *JACC Cardiovasc Interv* 2015;8:866-868.

No of figures: 3 (all colour)

Figure captions:

Figure 1. Identifying the valve view by EchoNavigator


Figure 2. Positioning of the Lotus valve using EchoNavigator.

Figure 3. Positioning of the Sapien 3 valve using EchoNavigator.

Figure 1 legend. After probe registration, a bi-plane echocardiographic view of the aortic valve is acquired. The annulus is marked in two perpendicular views. The Free view of EchoNavigator is rotated such that the annulus will look like a line, representing aligned aortic valve sinuses. The valve view is shown at the right lower corner of the screen.

Figure 2 legend. Fused real time 3D TEE image on the X-ray screen can be used for positioning of the TAVR valve in combination with fluoroscopy. Red line represents annulus, blue arrows: aortic valve leaflets, green arrow: Lotus valve radiopaque marker.

Figure 3 legend. Positioning of the Sapien 3 valve using fluoro-echo fusion imaging. Red arrows: aortic valve leaflets, blue arrow: Sapien valve radiopaque marker.

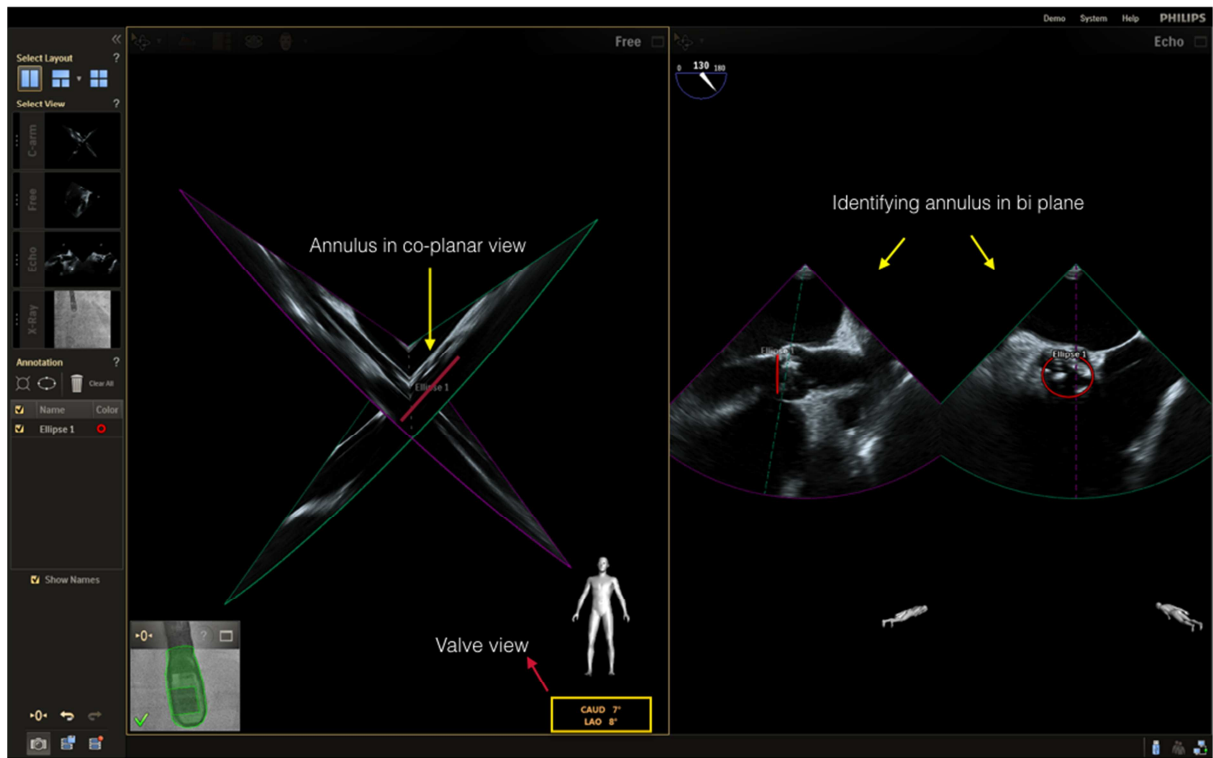

ACCEPTED MANUSCRIPT



ACCEPTED MANUSCRIPT

